


Appendix B

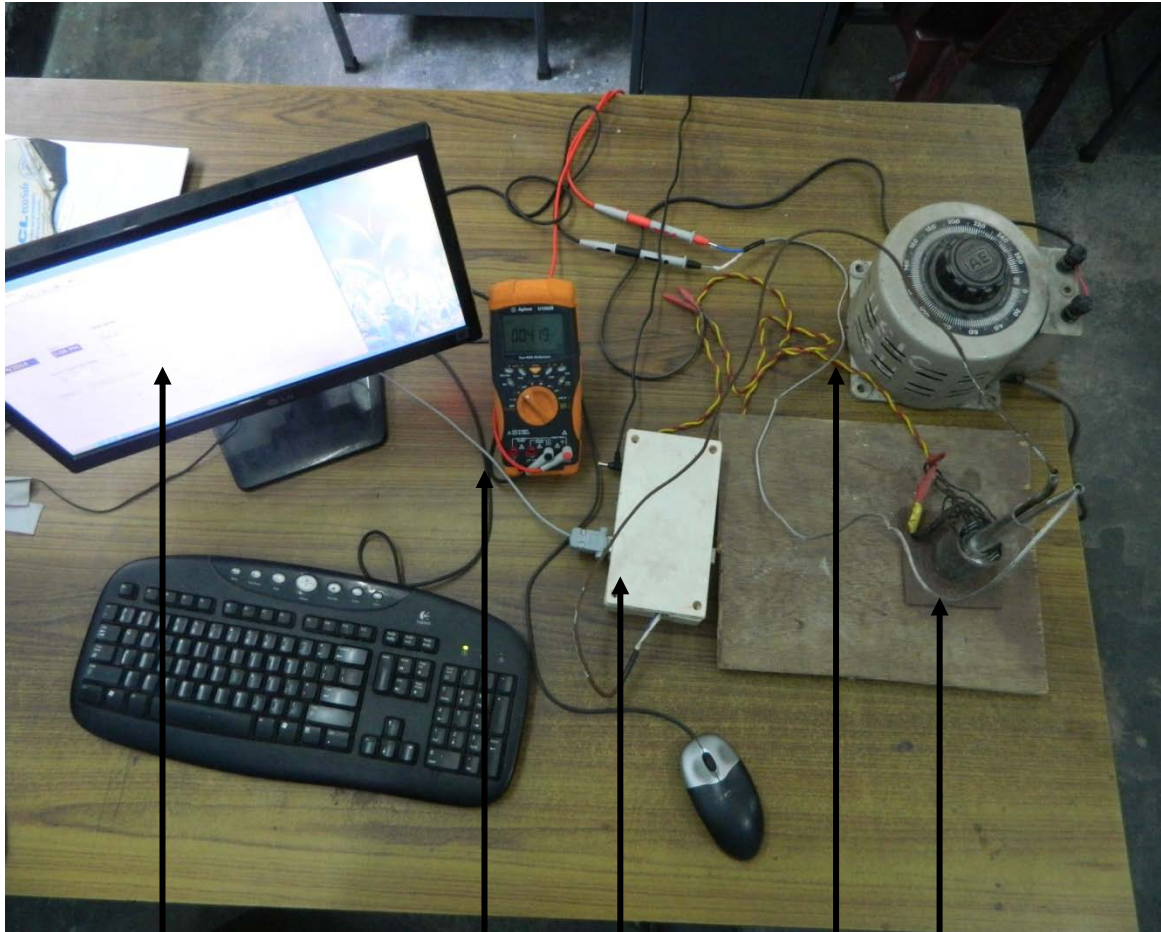

Data Acquisition
at PC


Digital
Multimeter

Sensor Node

Variac

Heating Chamber
with Thermocouple

B1: Calibration set-up of thermocouple based sensor node

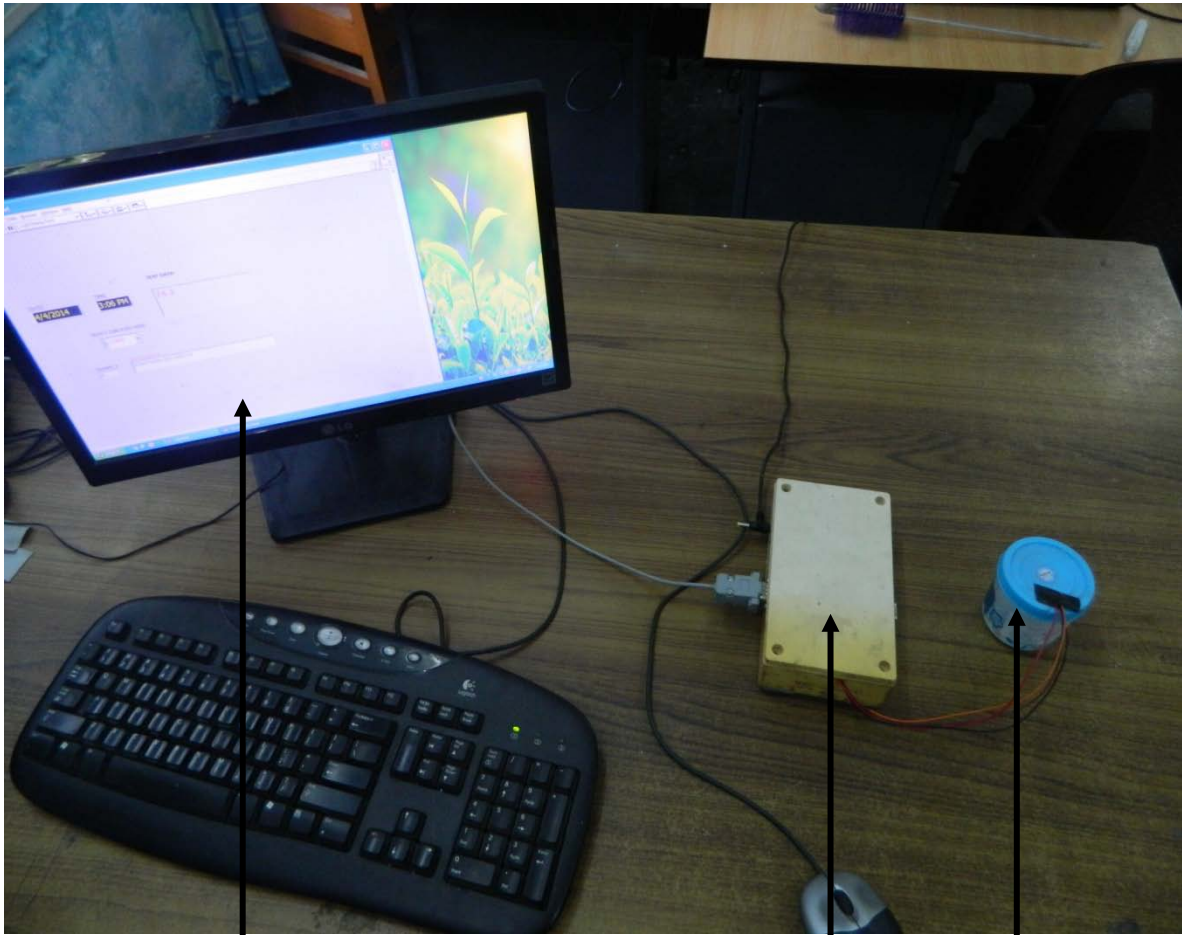

Data Acquisition
at PC

Binary Salt Solution
Chamber

Sensor Node

B2: Calibration set-up of Temperature and RH sensor node